



# M300 Series Data Acquisition/ Switch System

- Up to 320 switch channels per mainframe, save on cost of ownership
- Can be run without PC
- USB logging
- Interval scanning with storage of up to 100,000 time-stamped readings
- 8 kinds of cards supported
- 6½ digits DMM can be enabled/disabled in any of slots
- Standard SCPI commands
- Math statistics: AVG, MAX, MIN, SDEV
- 4.3' TFT LCD
- Powerful PC software
- Full Interfaces supported: USB Device,USB Host, GPIB, LAN(LXI-Core 2011 Device), RS232

M300 Series Data Acquisition/Switch System with modular structure, which combines precision measurement capability with flexible signal connections, can provide versatile solutions for the applications with multiple points or signals to be tested in product performance test during R&D phase as well as automatic test during production process.



## M300 Series Data Acquisition/Switch System



Product Dimensions: Width X Height X Depth=239.0mm×159.0 mm×373.4 mm Weight: 5.7 kg(Without Package)

## ► Feature and Benefits

- Channel Configuration Guide

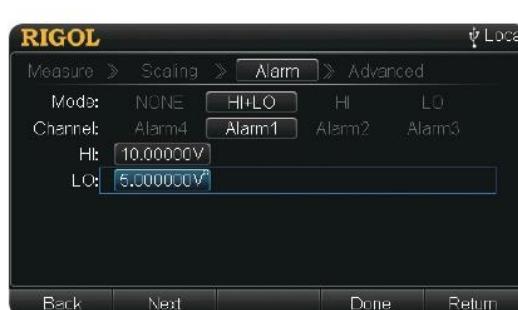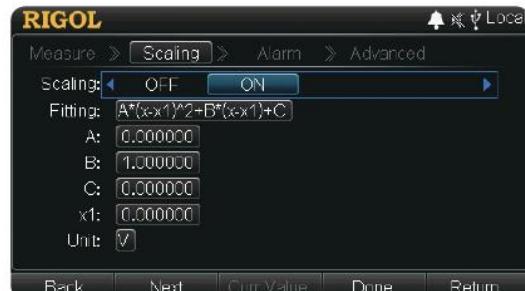

- Channel Monitor



Single Channel Monitor

Chan	Function	Range	Meas Value	Alarm
201	DCV	Auto	-1.217665mV	LO
202	DCV	Auto	-2.832402mV	LO
203	DCV	Auto	-2.499097mV	LO
204	DCV	Auto	-1.535608mV	LO
205	DCV	Auto	-2.307539mV	LO
206	DCV	Auto	-2.771090mV	LO
207	DCV	Auto	-2.857446mV	LO

Multiple/All Channel Monitor


- Multi-View Switch




Display real-time scan information and all the measurement data of the channel selected

101	102	103	104	105	106	107	108	109	110
111	112	113	114	115	116	117	118	119	120
121	122	123	124	125	126	127	128	129	130
131	132	133	134	135	136	137	138	139	140
141	142	143	144	145	146	147	148	149	150
151	152	153	154	155	156	157	158	159	160
161	162	163	164	201	202	203	204	205	206
207	208	209	210	211	212	213	214	215	216

Display real-time channel status

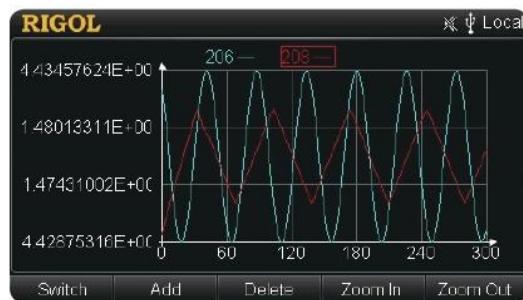

Draw scan data curves

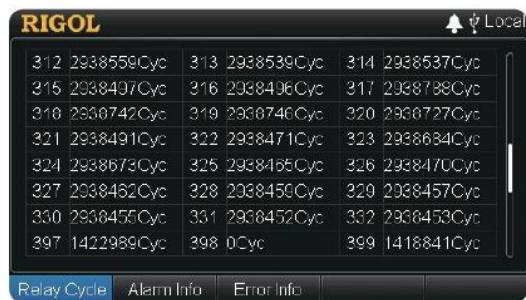

Record each relay cycle on each module




## Alarm Information



## Error Information

- Multiple Configuration Copy Functions

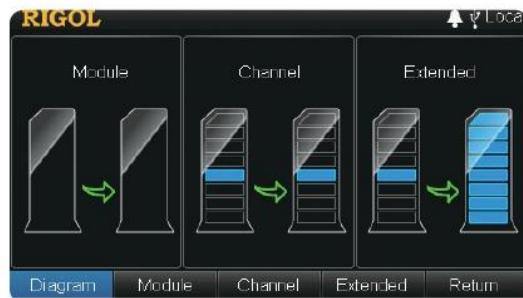

Multiple configuration copy function, can configure multiple channels conveniently and quickly



Module Conv



### Channel Copy




### Extended Copy

• To Control Each Module Separately



To control each module separately

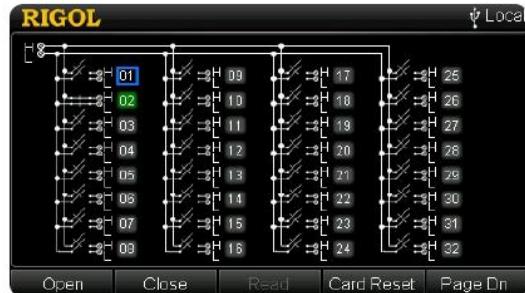


MC3132 Control Interface




MC3164 Control Interface



MC3648 Control Interface

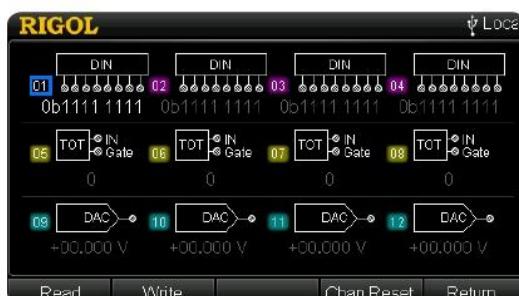


MC3534 Control Interface

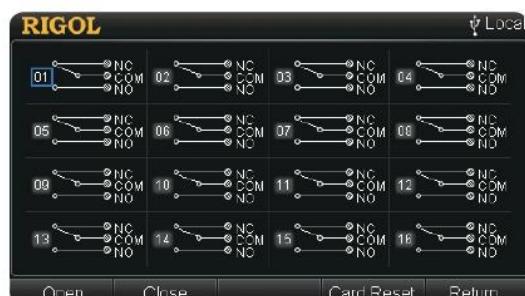


MC3416 Control Interface

- Channel Configuration of Ultra Acquire

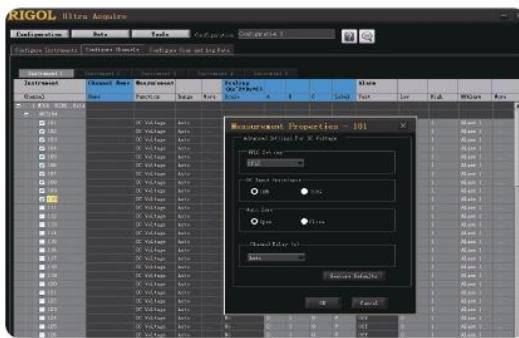

- Data Analysis of Ultra Acquire

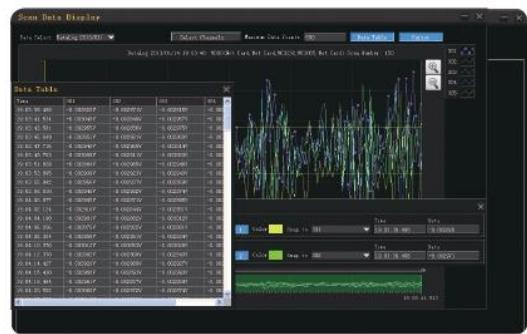

## ► Specifications

### DC Characteristics

Accuracy Specifications:  $\pm$  (% of reading + % of range)<sup>(1)</sup>

Function	Range <sup>(2)</sup>	Test Current or Load Voltage	24 Hour <sup>(3)</sup> $T_{cal}$ °C ± 1°C	90 Day $T_{cal}$ °C ± 5°C	1 Year $T_{cal}$ °C ± 5°C	Temperature Coefficient 0°C to ( $T_{cal}$ °C – 5°C) ( $T_{cal}$ °C + 5°C) to 50°C
DC Voltage	200.0000mV	–	0.0020 + 0.0020	0.0030 + 0.0025	0.0040 + 0.0025	0.0005 + 0.0005
	2.000000V	–	0.0015 + 0.0005	0.0020 + 0.0006	0.0035 + 0.0006	0.0005 + 0.0001
	20.00000V	–	0.0020 + 0.0004	0.0030 + 0.0005	0.0040 + 0.0005	0.0005 + 0.0001
	200.0000V	–	0.0020 + 0.0006	0.0040 + 0.0006	0.0050 + 0.0006	0.0005 + 0.0001
	300.000V	–	0.0020 + 0.0006	0.0040 + 0.0010	0.0055 + 0.0010	0.0005 + 0.0001
DC Current	200.000 μA	<0.03V	0.010 + 0.012	0.040 + 0.015	0.050 + 0.015	0.0020 + 0.0030
	2.000000mA	<0.25V	0.007 + 0.003	0.030 + 0.003	0.050 + 0.003	0.0020 + 0.0005
	20.00000mA	<0.07V	0.007 + 0.012	0.030 + 0.015	0.050 + 0.015	0.0020 + 0.0020
	200.0000mA	<0.7V	0.010 + 0.002	0.030 + 0.003	0.050 + 0.003	0.0020 + 0.0005
	1.000000A	<0.12V	0.050 + 0.020	0.080 + 0.020	0.100 + 0.020	0.0050 + 0.0010
Resistance <sup>(4)</sup>	200.0000Ω	1mA	0.0030 + 0.0030	0.008 + 0.004	0.010 + 0.004	0.0006 + 0.0005
	2.000000kΩ	1mA	0.0020 + 0.0005	0.008 + 0.001	0.010 + 0.001	0.0006 + 0.0001
	20.00000kΩ	100 μA	0.0020 + 0.0005	0.008 + 0.001	0.010 + 0.001	0.0006 + 0.0001
	200.0000kΩ	10 μA	0.0020 + 0.0005	0.008 + 0.001	0.010 + 0.001	0.0006 + 0.0001
	1.000000MΩ	2 μA	0.002 + 0.001	0.010 + 0.001	0.012 + 0.001	0.0010 + 0.0002
	10.00000MΩ	200nA	0.015 + 0.001	0.030 + 0.001	0.040 + 0.001	0.0030 + 0.0004
	100.0000MΩ	200nA    10MΩ	0.300 + 0.010	0.800 + 0.010	0.800 + 0.010	0.1500 + 0.0002

NOTE: (1) Specifications are for 90-minute warm-up and 100 PLC integration time.

(2) 10% overrange on all ranges.

(3) Relative to calibration standards.

(4) Specifications are for 4-wire resistance measurement. Add 3 Ω additional error in 2-wire resistance measurement.

### Measuring Characteristics

DC Voltage	
Input Impedance	200mV, 2V, 20V ranges: 10MΩ or >10GΩ (For these ranges, input beyond $\pm 26$ V are clamped through 106 kΩ)
	200V and 300V ranges: 10MΩ ± 1%
Input Protection	300V
Input Offset Current	50pA, at 25°C, typical
CMRR (common mode rejection ratio)	140 dB for 1 kΩ unbalanced resistance in LO lead, ± 300 VDC peak maximum.
Resistance	
Measurement Method	4-wire or 2-wire resistance Current source referenced to LO input
Open-circuit Voltage	Limited to <10 V
Max. Lead Resistance (4-wire)	10% of range per lead for 200 Ω and 2 kΩ ranges, 1 kΩ per lead on all other ranges
Input Protection	300V on all ranges
Offset Compensation	Available on 200 Ω, 2 kΩ and 20 kΩ ranges.
DC Current	
Shunt Resistor	100 Ω for 200 μA, 2 mA 1 Ω for 20 mA, 200 mA 0.1 Ω for 1 A

### Auto Zero OFF Operation (typical value)

Following instrument warm-up at the environment temperature  $\pm 1^\circ\text{C}$  and <5 minutes, add 0.0001 % range + 2 uV error for DCV and 2 mΩ error for resistance.

### Settling Considerations

Reading settling times are affected by source impedance, cable dielectric characteristics and input signal changes. The default measurement delay can ensure the correctness of the first reading for most measurements.

### Measurement Considerations

Teflon or other high-impedance, low-dielectric absorption wire insulation is recommended for these measurements.

## AC Characteristics

Accuracy Specifications:  $\pm$  (% of reading + % of range)<sup>11</sup>

Function	Range <sup>12</sup>	Frequency Range	24 Hour <sup>13</sup> $T_{CAL}^{\circ}\text{C} \pm 1^{\circ}\text{C}$	90 Day $T_{CAL}^{\circ}\text{C} \pm 5^{\circ}\text{C}$	1 Year $T_{CAL}^{\circ}\text{C} \pm 5^{\circ}\text{C}$	Temperature Coefficient $0^{\circ}\text{C}$ to ( $T_{CAL}^{\circ}\text{C} - 5^{\circ}\text{C}$ ) ( $T_{CAL}^{\circ}\text{C} + 5^{\circ}\text{C}$ ) to $50^{\circ}\text{C}$
True RMS AC Voltage <sup>14</sup>	200.0000mV	3Hz–5Hz	1.00 + 0.03	1.00 + 0.04	1.00 + 0.04	0.100 + 0.004
		5Hz–10Hz	0.35 + 0.03	0.35 + 0.04	0.35 + 0.04	0.035 + 0.004
		10Hz–20kHz	0.04 + 0.03	0.05 + 0.04	0.06 + 0.04	0.005 + 0.004
		20kHz–50kHz	0.10 + 0.05	0.11 + 0.05	0.12 + 0.05	0.011 + 0.005
		50kHz–100kHz	0.55 + 0.08	0.60 + 0.08	0.60 + 0.08	0.060 + 0.008
		100kHz–300kHz	4.00 + 0.50	4.00 + 0.50	4.00 + 0.50	0.20 + 0.02
	2.000000V	3Hz–5Hz	1.00 + 0.02	1.00 + 0.03	1.00 + 0.03	0.100 + 0.003
		5Hz–10Hz	0.35 + 0.02	0.35 + 0.03	0.35 + 0.03	0.035 + 0.003
		10Hz–20kHz	0.04 + 0.02	0.05 + 0.03	0.06 + 0.03	0.005 + 0.003
		20kHz–50kHz	0.10 + 0.04	0.11 + 0.05	0.12 + 0.05	0.011 + 0.005
		50kHz–100kHz	0.55 + 0.08	0.60 + 0.08	0.60 + 0.08	0.060 + 0.008
		100kHz–300kHz	4.00 + 0.50	4.00 + 0.50	4.00 + 0.50	0.20 + 0.02
	20.00000V	3Hz–5Hz	1.00 + 0.03	1.00 + 0.04	1.00 + 0.04	0.100 + 0.004
		5Hz–10Hz	0.35 + 0.03	0.35 + 0.04	0.35 + 0.04	0.035 + 0.004
		10Hz–20kHz	0.04 + 0.04	0.07 + 0.04	0.08 + 0.04	0.008 + 0.004
		20kHz–50kHz	0.10 + 0.05	0.12 + 0.05	0.15 + 0.05	0.012 + 0.005
		50kHz–100kHz	0.55 + 0.08	0.60 + 0.08	0.60 + 0.08	0.060 + 0.008
		100kHz–300kHz	4.00 + 0.50	4.00 + 0.50	4.00 + 0.50	0.20 + 0.02
	200.0000V	3Hz–5Hz	1.00 + 0.02	1.00 + 0.03	1.00 + 0.03	0.100 + 0.003
		5Hz–10Hz	0.35 + 0.02	0.35 + 0.03	0.35 + 0.03	0.035 + 0.003
		10Hz–20kHz	0.04 + 0.02	0.07 + 0.03	0.08 + 0.03	0.008 + 0.003
		20kHz–50kHz	0.10 + 0.04	0.12 + 0.05	0.15 + 0.05	0.012 + 0.005
		50kHz–100kHz	0.55 + 0.08	0.60 + 0.08	0.60 + 0.08	0.060 + 0.008
		100kHz–300kHz	4.0 + 0.50	4.0 + 0.50	4.0 + 0.50	0.20 + 0.02
	300.000V	3Hz–5Hz	1.00 + 0.02	1.00 + 0.03	1.00 + 0.03	0.100 + 0.003
		5Hz–10Hz	0.35 + 0.02	0.35 + 0.03	0.35 + 0.03	0.035 + 0.003
		10Hz–20kHz	0.04 + 0.02	0.07 + 0.03	0.08 + 0.03	0.008 + 0.003
		20kHz–50kHz	0.10 + 0.04	0.12 + 0.05	0.15 + 0.05	0.012 + 0.005
		50kHz–100kHz	0.55 + 0.08	0.60 + 0.08	0.60 + 0.08	0.060 + 0.008
		100kHz–300kHz	4.0 + 0.50	4.0 + 0.50	4.0 + 0.50	0.20 + 0.02
True RMS AC Current <sup>15</sup>	200.0000 $\mu\text{A}$	3Hz–5Hz	1.10 + 0.06	1.10 + 0.06	1.10 + 0.06	0.200 + 0.006
		5Hz–10Hz	0.35 + 0.06	0.35 + 0.06	0.35 + 0.06	0.100 + 0.006
		10Hz–5kHz	0.15 + 0.06	0.15 + 0.06	0.15 + 0.06	0.015 + 0.006
		5kHz–10kHz	0.35 + 0.70	0.35 + 0.70	0.35 + 0.70	0.030 + 0.006
	2.000000mA	3Hz–5Hz	1.00 + 0.04	1.00 + 0.04	1.00 + 0.04	0.100 + 0.006
		5Hz–10Hz	0.30 + 0.04	0.30 + 0.04	0.30 + 0.04	0.035 + 0.006
		10Hz–5kHz	0.12 + 0.04	0.12 + 0.04	0.12 + 0.04	0.015 + 0.006
		5kHz–10kHz	0.20 + 0.25	0.20 + 0.25	0.20 + 0.25	0.030 + 0.006
	20.00000mA	3Hz–5Hz	1.10 + 0.06	1.10 + 0.06	1.10 + 0.06	0.200 + 0.006
		5Hz–10Hz	0.35 + 0.06	0.35 + 0.06	0.35 + 0.06	0.100 + 0.006
		10Hz–5kHz	0.15 + 0.06	0.15 + 0.06	0.15 + 0.06	0.015 + 0.006
		5kHz–10kHz	0.35 + 0.70	0.35 + 0.70	0.35 + 0.70	0.030 + 0.006
	200.0000mA	3Hz–5Hz	1.00 + 0.04	1.00 + 0.04	1.00 + 0.04	0.100 + 0.006
		5Hz–10Hz	0.30 + 0.04	0.30 + 0.04	0.30 + 0.04	0.035 + 0.006
		10Hz–5kHz	0.10 + 0.04	0.10 + 0.04	0.10 + 0.04	0.015 + 0.006
		5kHz–10kHz	0.20 + 0.25	0.20 + 0.25	0.20 + 0.25	0.030 + 0.006
	1.000000A	3Hz–5Hz	1.10 + 0.06	1.10 + 0.06	1.10 + 0.06	0.100 + 0.006
		5Hz–10Hz	0.35 + 0.06	0.35 + 0.06	0.35 + 0.06	0.035 + 0.006
		10Hz–5kHz	0.15 + 0.06	0.15 + 0.06	0.15 + 0.06	0.015 + 0.006
		5kHz–10kHz	0.35 + 0.70	0.35 + 0.70	0.35 + 0.70	0.030 + 0.006
		5Hz–10Hz	0.35 + 0.08	0.35 + 0.10	0.35 + 0.10	0.035 + 0.008
		10Hz–5kHz	0.15 + 0.08	0.15 + 0.10	0.15 + 0.10	0.015 + 0.008

NOTE: [1] Specifications are for 90–minute warm-up, slow ac filter and sine wave input.

[2] 10% overrange on all ranges.

[3] Relative to calibration standards.

[4] Specifications are for sine wave input >5% of range. For inputs from 1% to 5% of range and <50 kHz, add 0.1% of range additional error. For 50 kHz to 100 kHz, add 0.13% of range.

[5] Specifications are for sine wave input >5% of range. For inputs from 1% to 5% of range, add 0.1% of range additional error.

Specifications are typical values for 200  $\mu\text{A}$ , 2 mA and 1 A ranges when frequency is >1 kHz.

## Measuring Characteristics

True RMS AC Voltage	
Measurement Method	AC-coupled True-RMS — measure the ac component of input with up to 300 V DC bias on any range.
Crest Factor	$\leq 5$ at full range
Input Impedance	$1 \text{ M}\Omega \pm 2\%$ , in parallel with $<150 \text{ pF}$ capacitance on any range
Input Protection	300 V rms on all ranges
AC Filter Bandwidth	Slow: 3 Hz – 300 kHz Medium: 20 Hz – 300 kHz Fast: 200 Hz – 300 kHz
CMRR (common mode rejection ratio)	70 dB, for the $1 \text{ k}\Omega$ unbalance in LO lead, <60 Hz common mode signal frequency, $\pm 300 \text{ VDC}$ peak maximum.
True RMS AC Current	
Measurement Method	Direct coupled to the fuse and shunt; AC-coupled True RMS measurement (measure the AC component).
Crest Factor	$\leq 3$ at full range
Max. Input	DC + AC current peak value $<300\%$ of range. Current with DC current component $<1 \text{ A rms}$ .
Shunt Resistor	100 $\Omega$ for 200 $\mu\text{A}$ , 2 mA 1 $\Omega$ for 20 mA, 200 mA 0.1 $\Omega$ for 1 A

### Settling Time Considerations

The default measurement delay of the multimeter can ensure the correctness of the first readings of most of the measurements. Make sure the RC circuit of input terminal has been fully settled (about 1 s) before accurate measurement.

## Frequency and Period Characteristics

Accuracy Specifications: $\pm (\% \text{ of reading})^{11112}$						
Function	Range	Frequency Range	24 Hour <sup>11</sup> $T_{\text{CAL}} \text{ }^{\circ}\text{C} \pm 1 \text{ }^{\circ}\text{C}$	90 Day $T_{\text{CAL}} \text{ }^{\circ}\text{C} \pm 5 \text{ }^{\circ}\text{C}$	1 Year $T_{\text{CAL}} \text{ }^{\circ}\text{C} \pm 5 \text{ }^{\circ}\text{C}$	Temperature Coefficient $0 \text{ }^{\circ}\text{C}$ to $(T_{\text{CAL}} \text{ }^{\circ}\text{C} - 5 \text{ }^{\circ}\text{C})$ $(T_{\text{CAL}} \text{ }^{\circ}\text{C} + 5 \text{ }^{\circ}\text{C})$ to $50 \text{ }^{\circ}\text{C}$
Frequency, Period	200mV–300V	3 Hz–5 Hz	0.07	0.07	0.07	0.005
		5 Hz–10 Hz	0.04	0.04	0.04	0.005
		10 Hz–40 Hz	0.02	0.02	0.02	0.001
		40 Hz–300 kHz	0.005	0.006	0.007	0.001
		300 kHz–1 MHz	0.005	0.006	0.007	0.001

### Additional Low Frequency Errors: (% of reading)

Frequency		Gate Time (Resolution)			
		1s ( 0.1ppm )	0.1s ( 1ppm )	0.01s ( 10ppm )	0.001s ( 100ppm )
3 Hz–5Hz	0	0	0.12	0.12	0.12
5 Hz–10Hz	0	0	0.17	0.17	0.17
10 Hz–40Hz	0	0	0.20	0.20	0.20
40 Hz–100Hz	0	0	0.06	0.21	0.21
100 Hz–300Hz	0	0	0.03	0.21	0.21
300 Hz–1 kHz	0	0	0.01	0.07	0.07
>1kHz	0	0	0	0.02	0.02

NOTE: 111 Specifications are for 90 minutes warm-up and 1 s gate time.

121 For frequency  $\leq 300$  kHz, the specification is for AC input voltage of 10% to 110% of range. For frequency  $>300$  kHz, the specification is for AC input voltage of 20% to 110% of range. The maximum input is limited to 750 Vrms or  $B \times 10^7$  Volts-Hz (whichever is less). 200 mV range is full range input or input that is larger than the full range.

For 20 mV to 200 mV inputs, multiply % of reading error by 10.

131 Relative to calibration standards.

## Measuring Characteristics

Frequency and Period	
Measurement Method	Reciprocal-counting technique, AC-coupled input using the AC voltage function.
Input Impedance	$1 \text{ M}\Omega \pm 2\%$ , in parallel with $<150 \text{ pF}$ capacitance on any range
Input Protection	300 Vrms on all ranges
Measurement Considerations	
All frequency counters are susceptible to error when measuring low-voltage, low-frequency signals. Shielding inputs from external noise pickup is critical for minimizing measurement errors.	
Settling Considerations	
Errors will occur when attempting to measure the frequency or period of an input following a dc offset voltage change. The input blocking RC time constant must be allowed to fully settle (about 1 s) before the most accurate measurements are possible.	

## Temperature Characteristics

Accuracy Specifications<sup>[1]</sup>

Function	Probe Type	Type	Optimum Range	1 Year $T_{CAL}^{\circ}\text{C} \pm 5^{\circ}\text{C}$	Temperature Coefficient 0°C to ( $T_{CAL}^{\circ}\text{C} - 5^{\circ}\text{C}$ ) ( $T_{CAL}^{\circ}\text{C} + 5^{\circ}\text{C}$ ) to 50°C
Temperature	RTD <sup>[2]</sup> (R <sub>0</sub> is within 49 Ω and 2.1 kΩ)	$\alpha = 0.00385$	-200°C – 660°C	0.16°C	0.01°C
		$\alpha = 0.00389$	-200°C – 660°C	0.17°C	0.01°C
		$\alpha = 0.00391$	-200°C – 660°C	0.14°C	0.01°C
		$\alpha = 0.00392$	-200°C – 660°C	0.15°C	0.01°C
	Thermal Resistance	2.2 kΩ	-40°C – 150°C	0.08°C	0.002°C
		3 kΩ	-40°C – 150°C	0.08°C	0.002°C
		5 kΩ	-40°C – 150°C	0.08°C	0.002°C
		10 kΩ	-40°C – 150°C	0.08°C	0.002°C
		30 kΩ	-40°C – 150°C	0.08°C	0.002°C
	Thermocouple <sup>[3]</sup>	B	0°C – 1820°C	0.76°C	0.14°C
		E	-270°C – 1000°C	0.5°C	0.02°C
		J	-210°C – 1200°C	0.5°C	0.02°C
		K	-270°C – 1372°C	0.5°C	0.03°C
		N	-270°C – 1300°C	0.5°C	0.04°C
		R	-50°C – 1768.1°C	0.5°C	0.09°C
		S	-50°C – 1768.1°C	0.6°C	0.11°C
		T	-270°C – 400°C	0.5°C	0.03°C

NOTE: [1] Specifications are for 90 minutes warm-up. Probe error excluded.

[2] Specification is for 4WR resistance measurement.

[3] Relative to cold junction temperature, accuracy is based on ITS-90. Built-in cold junction temperature refers to the temperature of the connector inside the terminal block and its accuracy is ± 2.5 °C.

## Measuring Characteristics

Thermocouple	
Conversion	ITS-90 software compensation
Reference Junction Type	Internal, Fixed, or External
T/C Check	Selectable per channel. When the channel resistance is >5kΩ, it is considered as Open.
RTD	
Alpha	= 0.00385 (DIN/IEC 751); using ITS-90 software compensation; = 0.00389, 0.00391 or 0.00392; using IPTS-68 software compensation
Thermistor	44004, 44007, 44006 series

## Measurement Considerations

The built-in cold junction temperature tracks the temperature inside the terminal box. The change of temperature in the terminal box might cause additional error. When using the built-in cold junction compensation, connect the sensor terminal of the thermocouple to the terminal box and warm it up for more than 3 minutes to minimize the error.

## Module Specifications

MC3120/MC3132/MC3164/MC3324/MC3416/MC3648

General	Multiplexer				Actuator	Matrix
	MC3120	MC3132	MC3164	MC3324	MC3416	MC3648
Number of Channels	20	32	64	20 Voltage+4 Current	16	4 x 8
2-wire mode or 4-wire mode <sup>[1]</sup>	2-wire mode or 4-wire mode <sup>[1]</sup>	2-wire mode or 4-wire mode <sup>[1]</sup>	1-wire mode <sup>[2]</sup>	2-wire mode or 4-wire mode <sup>[3]</sup>	SPDT	2-wire mode
Connect to DMM Module?	Yes	Yes	Yes	Yes	No	No
Scanning Speed <sup>[4]</sup>	60Ch/s	60Ch/s	60Ch/s	60Ch/s	—	—
Open/Close Speed	200Ch/s	200Ch/s	200Ch/s	200Ch/s	200Ch/s	200Ch/s
Maximum Input						
Voltage (DC, AC rms)	300Vrms	300Vrms	300Vrms	300Vrms	300Vrms	300Vrms
Current (DC, AC rms)	1Arms	1Arms	1Arms	1Arms	2Arms	1Arms
Power (W, VA)	50VA	50VA	50VA	50VA	60VA	50VA
Isolation (ch-ch, ch-earth) (DC, AC rms)	300Vrms	300Vrms	300Vrms	300Vrms	300Vrms	300Vrms
DC Characteristics						
Offset Voltage	5uV	5uV	5uV	5uV	<3uV	5uV
Initial Closed Channel Resistance	<1Ω	<1Ω	<1Ω	<1Ω	<0.1Ω	<1Ω
Isolation (ch-ch, ch-earth)	>10GΩ	>10GΩ	>10GΩ	>10GΩ	>10GΩ	>10GΩ
AC Characteristics						
Bandwidth	1MHz	1MHz	1MHz	1MHz	1MHz	1MHz
Ch-Ch Cross Talk (dB) <sup>[5]</sup> 1MHz	-45	-45	-18 <sup>[6]</sup>	-45	-15	-18
Capacitance HI-LO	100pF	100pF	100pF	100pF	<500pF	100pF
Capacitance LO-Earth	200pF	200pF	200pF	200pF	<200pF	200pF
Volt-Hertz Limit	10 <sup>8</sup>	10 <sup>8</sup>	10 <sup>8</sup>	10 <sup>8</sup>	10 <sup>8</sup>	10 <sup>8</sup>
Other						
T/C Cold Junction Accuracy (Typical)	0.8°C	0.8°C	0.8°C <sup>[7]</sup>	0.8°C	—	—
Switch Life (No Load) (Typical)	100M	100M	100M	100M	100M	100M
Switch Life (Rated Load) (Typical) <sup>[8]</sup>	100K	100K	100K	100K	100K	100K
Operating Temperature	0°C – 55°C	0°C – 55°C	0°C – 55°C	0°C – 55°C	0°C – 55°C	0°C – 55°C
Storage Temperature	-20°C – 70°C	-20°C – 70°C	-20°C – 70°C	-20°C – 70°C	-20°C – 70°C	-20°C – 70°C
Humidity (non-condensing)	40°C / 80% RH	40°C / 80% RH	40°C / 80% RH	40°C / 80% RH	40°C / 80% RH	40°C / 80% RH

NOTE: [1] 20 channel multiplexer can be used as 20 2-wire or 10 4-wire measurement channels and 32 channel multiplexer can be used as 32 2-wire or 16 4-wire measurement channels.

[2] 64 channel multiplexer share a Common Low for two banks of 32 channels.

[3] 24 Channel multiplexer can be configured as 20 2-wire voltage channels or 10 4-wire voltage channels in addition to the 4 current channels.

[4] Integration time: 0.02PLC, channel delay: 0, auto zero: off, alarm: off, scaling: off, data to internal memory (disconnect the communication of the LAN, USB, GPIB or RS232 interface), the results are measured under the DCV function.

[5] 50Ω load.

[6] Isolation within banks is -40dB.

[7] Specifications are for the LO setting and not the temperature of the cold terminal.

[8] Applies to resistive loads only.

## MC3534

Digital Input/Output (DIO)								
Port 1,2,3,4	8-bit, input or output, non-isolated							
Type	Vin(L)	Vin(H)	Vout(L)	Vout(H)	Vin(H) Max			
TTL	<0.8V	>2.0V	<0.2V@I <sub>out</sub> =-500mA	>4.8V@I <sub>out</sub> =1mA	<42V with external open drain pull-up			
5V CMOS	<1.5V	>3.5V	<0.2V@I <sub>out</sub> =-500mA	>4.8V@I <sub>out</sub> =1mA				
3.3V CMOS	<1.0V	>2.3V	<0.2V@I <sub>out</sub> =-500mA	>3.15V@I <sub>out</sub> =1mA				
2.5V CMOS	<0.75V	>1.75V	<0.2V@I <sub>out</sub> =-500mA	>2.35V@I <sub>out</sub> =1mA				
User defined	Threshold-0.3V	Threshold+0.3V	<0.2V@I <sub>out</sub> =-500mA	>(Level-0.2V)@I <sub>out</sub> =1mA				
Alarming	Match or mismatch, maskable				Match or mismatch, maskable			
Speed	4ms (Max) alarm sampling				4ms (Max) alarm sampling			
Latency	5ms				5ms			
Read/Write Speed	100/s				100/s			
Totalizer Input (TOT)								
	High Speed (TOT1,TOT2)		Normal Speed (TOT3,TOT4)					
Maximum Count	2 <sup>32</sup> -1		2 <sup>32</sup> -1					
Totalizer Input	10MHz (max), rising or falling edge, programmable		100kHz (max), rising or falling edge, programmable					
Signal Level	CMOS 3.3V,5V tolerable		1V <sub>p-p</sub> (min),42V <sub>pk</sub> (max), V <sub>cm</sub> =-12V~+12V					
Threshold	Fixed at CMOS 3.3V		-12V~+12V, Programmable					
Gated Input	CMOS 3.3V-Hi, CMOS 3.3V-Lo or none, 5V tolerance		CMOS 3.3V-Hi, CMOS 3.3V-Lo or none, 5V tolerance					
Count Reset	Manual or Read + Reset		Manual or Read + Reset					
Read Speed	100/s		100/s					
Analog Voltage Output (DAC)								
DAC 1,2,3,4	$\pm 12V$ , non-isolated (earth referenced)							
Resolution	1mV							
I <sub>out</sub>	10mA max							
Setting Time	1ms to 0.01 % of output							
Accuracy	$\pm (\% \text{ of output} + \text{mV})$							
1 year $\pm 5^\circ\text{C}$	0.25%+20mV							
Temp Coefficient	$\pm (0.015\% + 1\text{mV})/\text{ }^\circ\text{C}$							

## General Specifications

Display	4.3 inches
Power Supply	AC 100V – 120V, 45Hz – 440Hz AC 200V – 240V, 45Hz – 66Hz Detect the power frequency automatically at power-on, 400 Hz defaults to 50 Hz
Power Consumption	25 VA Max
Working Environment	Full accuracy for 0°C to 50°C Full accuracy to 80% R.H. at 40°C Non-coagulation
Storage Temperature	-40°C to 70°C
Operation Altitude	Up to 2000 meters
Safety	IEC 61010-1; EN 61010-1; UL 61010-1; CAN/CSA-C22.2 No. 61010-1 Measurement CAT I 300V Pollution Degree 2
EMC	EN 61326-1
Weight	About 5.7 kg (without package)
Dimension	(height × width × length): 159.0mm × 239.0mm × 373.4mm
Remote Interface	GPIB, 10/100Mbit LAN, USB 2.0 Full Speed Device & Host (support USB storage device), RS232
Programming Language	SCPI
LXI Compatibility	LXI Core 2011 Device, Version 1.4
Warm-up Time	90 minutes